

## Research Article

# Role of Sonoelastography in Differentiating Benign and Malignant Salivary Gland Tumors: A Systematic Review and Meta Analysis

Mahsa Ghajarzadeh<sup>1\*</sup>, Mehdi Mohammadifar<sup>2</sup> and Seyed Hassan Emami-Razavi<sup>1</sup>

<sup>1</sup>Brain and Spinal Injury Research Center, Tehran University of Medical Sciences, Iran

<sup>2</sup>Department of Radiology, Zanzan University of Medical Sciences, Iran

\*Corresponding author: Mahsa Ghajarzadeh, Brain and Spinal Injury Research Center, Tehran University of Medical Sciences, Tehran, Iran

Received: October 21, 2015; Accepted: January 31, 2016; Published: March 01, 2016

## Abstract

**Objective:** The goal of this systematic review is to determine the diagnostic accuracy of sonoelastography in evaluating salivary gland tumors.

**Data sources:** A highly sensitive search for sonoelastography and salivary gland tumors was performed through MEDLINE, Cochrane Library, ACP Journal Club, EMBASE, Health Technology assessment, and ISI web of knowledge for studies published prior to January 2013.

A manual search was performed to include additional studies from references of the retrieved articles.

**Review methods:** Two independent reviewers evaluated articles for eligibility. They extracted data from included studies.

The quality of included studies was evaluated by use of Quality Assessment of Diagnostic Accuracy Studies (QUADAS) questionnaire which consists of 14, four option questions (yes, no, unclear, Not Applicable (N/A)).

Forest plots for pooled estimates and summary of ROC plots for different cut-offs were produced.

**Results:** The literature review and manual search yielded 15 articles, 6 of which eligible to be included. A total of 348 individuals with total number of 366 salivary gland masses were evaluated. Eighty seven were malignant while, 269 were benign. Three hundred and twenty two were located in parotid gland and forty four were in sub-mandibular gland.

The summary sensitivity and specificity for the differentiation of benign and malignant salivary gland masses were 0.63 and 0.59. The summary Diagnostic OR (D OR), positive and negative LR were 3.18, 1.63 and 0.61. The Area Under the Curve (AUC) was 0.68 (SE=0.03).

**Conclusion:** Sono-elastography had moderate accuracy in differentiating benign from malignant salivary gland tumors.

**Keywords:** Sonoelastography; Salivary gland tumors

## Introduction

Salivary gland tumors count near 3% of all head and neck tumors [1] which could locate in major or minor salivary glands. The incidence rate of these tumors has been reported between 1 to 5 cases per 100000 person [1,2].

The initial imaging modality applied for salivary gland masses is sonography as it is cost-effective, non invasive and easy to apply [3].

By means of B-mode and color Doppler evaluation, echogenicity, structure, size, contour, calcification and vascularity could be examined, although previous studies demonstrated that the accuracy of these parameters for differentiating benign and malignant lesions are not satisfactory [4-6].

Elastography is a new sonographic modality which provides data regarding tissue stiffness. It provides tissue elasticity estimation by

means of local compression.

Under external forces, soft tissues move more than harder ones and reflecting that malignant tissues are firmer than surrounding benign counterparts [7].

Series of previous studies had evaluated accuracy of sonoelastography in differentiating benign and malignant salivary gland tumors. Its sensitivity and specificity had been reported ranging from 41% to 75% and 47% to 91%, respectively [3,7-11].

The goal of this study was to perform a meta-analysis of published information to evaluate the overall accuracy of sonoelastography for differentiation of benign and malignant salivary gland tumors.

## Materials and Methods

We searched MEDLINE, Cochrane Library, EMBASE, ACP Journal Club, Health Technology Assessment, and ISI web of

**Table 1:** Characteristics of the included studies.

Author	Publication year	Mean age	Total number of patients	Male/female	Total number of masses	Malignant /Benign	Parotid/ submandibular	Method of classification
Bhatia	2010	60	61	48/13	65	6/59	57/8	Scoring system (1-4)
Dumitriu	2011	50	66	37/29	74	18/56	63/11	Scoring system (1-4)
Yerli	2012	49	46	N/A	36	8/28	30/6	Scoring system (1-4)
Wierzbicka	2012	54	43	16/27	43	10/33	43/0	Scoring system (1-5) and strain ratio
Celebi	2012	47	75	36/39	81	32/49	81/0	Scoring system (1-4)
Dumitriu	2010	50	57	N/A	57	13/44	48/9	Strain ratio

**Table 2:** Quality assessment of included studies.

Author	Q1 Spectm composition	Q2 Selecton criteria	Q3 Appropriate reference standard	Q4 Disease Progression bias	Q5 Partial verification bias	Q6 Differential verification bias	Q7 Incorporation bias	Q8 Test execution details	Q9 Reference execution details	Q10 Test review bias	Q11 Diagnostic review bias	Q12 Clinical review bias	Q13 Intermediate results	Q14 Withdrawals
Bhatia	Yes s	yes	Yes	Yes	Yes	Yes	Yes	Yes	Yes	Yes	Yes	Yes	Un clear	Un clear
Dumitru	Yes	Yes	Yes	No	Yes	Yes	Yes	Yes	Yes	Yes	Un clear	Un clear	Un clear	Un clear
Yerli	Yes	Yes	Yes	No	Yes	Yes	Yes	Yes	Yes	Un clear	Un clear	Yes	Un clear	Un clear
Wierzbicka	Yes	Yes	Yes	No	Yes	Yes	Yes	Yes	Yes	Un clear	Un clear	Yes	Un clear	Un clear
Celebi	Yes	Yes	Yes	Un clear	Un clear	Yes	Yes	Yes	Yes	Un clear	Un clear	Yes	Un clear	Un clear
Dumitru	Yes	Yes	Yes	Un clear	Un clear	Yes	Yes	Yes	Yes	Un clear	Un clear	Yes	Un clear	Un clear

**Table 3:** Summary estimates of sonoelastography.

	(95%CI)
Sensitivity	0.63 (0.52-0.73)
Specificity	0.59(0.53-0.65)
Diagnostic OR (DOR)	3.18(1.86-5.44)
Positive LR	1.63(1.33-2.01)
Negative LR	0.61(0.47-0.79)

knowledge for studies published prior to December 10<sup>th</sup>, 2012 by using these search terms: “elastography“, “sonoelastography“, “real-time tissue elastography“, “elasticity“, “elastogram“, “elasticity imaging techniques“, “salivary gland“, “neoplasm“, “tumor“, “carcinoma”.

A manual search was performed to include additional studies from references of the retrieved articles. Two independent reviewers evaluated articles for eligibility. The criteria for eligibility were:

1. Studies evaluated diagnostic accuracy of sonoelastography in differentiating malignant and benign salivary gland tumors. Systematic review articles, narrative review articles, letter to editors and editorial articles were excluded.
2. Using appropriate reference standard test such as Fine-Needle Aspiration (FNA), histological assessment of specimens obtained by surgery or dissection.
3. Diagnostic measures on sonoelastographic evaluation results such as sensitivity, specificity, positive and negative predictive values.

**Data extraction and quality assessment**

Two independent reviewers extracted data from included studies. Extracted data included: first author name, study publication year, country, number of patients, number of malignant and benign salivary masses, mean patient age in each study, number of male and female patients, classification method, number of parotid or submandibular masses.

The quality of included studies was evaluated by means of Quality Assessment of Diagnostic Accuracy Studies (QUADAS) questionnaire which consists of 14, four option questions (yes, no, unclear, Not Applicable (N/A)). The same two independent reviewers evaluated the quality of studies and in discord cases, disagreement solved by consensus of reviewers.

**Statistical analysis and data synthesis**

Accuracy of sonoelastography method was assessed by pooled estimates of sensitivity, specificity, positive and negative predictive values, and diagnostic odds ratio. In case of homogeneity, fixed-effect model applied for pooled estimate calculation and if significant heterogeneity was present, the random-effect model was used .The Cochran Q test was estimated to detect the heterogeneity among studies. Inconsistency (I<sup>2</sup>) was calculated to describe the percentage of the variability attributable to heterogeneity.

Summary Receiver Operating Characteristic (SROC) curves were constructed, by means of Moses-Shapiro-Littenberg method and the Area Under the Curve (AUC) was calculated. P Value of <0.05 was considered significant.

**Results**

The chart describes the fellow of study selection in this systematic review. The literature and manual search yielded 15 articles, of which, 6 were eligible to include in this study which were published between 2010 and 2012. The studies were conducted in Poland (N=1), Romania (N=2), Turkey (N=2) and China Union (N=1).

A total of 348 individuals with total number of 366 salivary gland masses were evaluated. Eighty seven were malignant while, 269 were benign. Three hundred and twenty two were located in parotid gland and forty four were in sub-mandibular gland.

In five studies, only qualitative scoring system (in four articles scoring 1-4) was used. In one study only strain ratios applied for

classification and in remaining one study, both strain ratio and elasticity scoring system (1-5) were applied.

Four studies used 1-4 scoring system while one used 1-5 and one strain ratio.

The characteristics of included articles are listed in (Table 1).

**Quality assessment of included studies**

Quality of included studies was evaluated by means of QUADAS questionnaire and information is present in (Table 2).

The summary sensitivity and specificity for the differentiation of benign and malignant salivary gland masses were 0.63 and 0.59. The summary Diagnostic OR (D OR), positive and negative LR were 3.18, 1.63 and 0.61 (Table 3).

**Test of heterogeneity**







All measurements showed homogeneity ( $I^2 < 50%$ ) in differentiating benign and malignant salivary gland masses except specificity ( $I^2 > 50%$ ).

**Discussion**

This is the first systematic review evaluating diagnostic accuracy of sonoelastography in differentiating benign and malignant salivary gland tumors.

The results of current study demonstrated that sonoelastography has modest accuracy in differentiating benign and malignant salivary gland tumors. The pooled sensitivity was 63% and pooled specificity was 59%. The summary diagnostic OR was 3.18 which could be indicative that the odds of obtaining a test positive result in malignant rather than benign tumors is three.

Salivary gland tumors form a wide group of masses which could locate in major or minor salivary glands. It is crucial to determine if

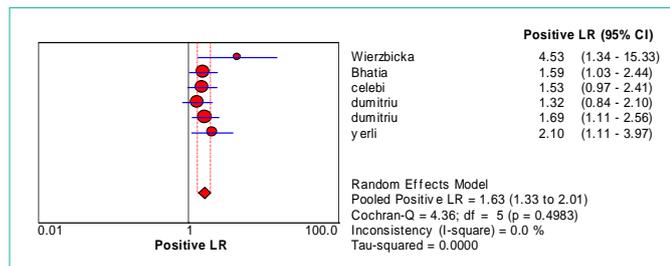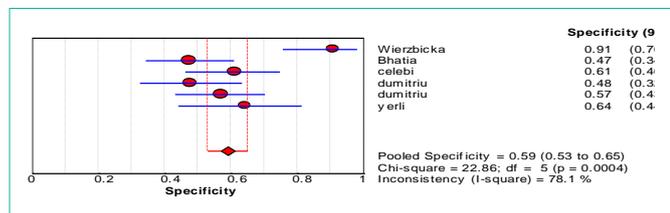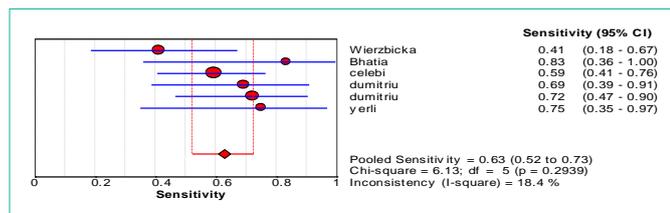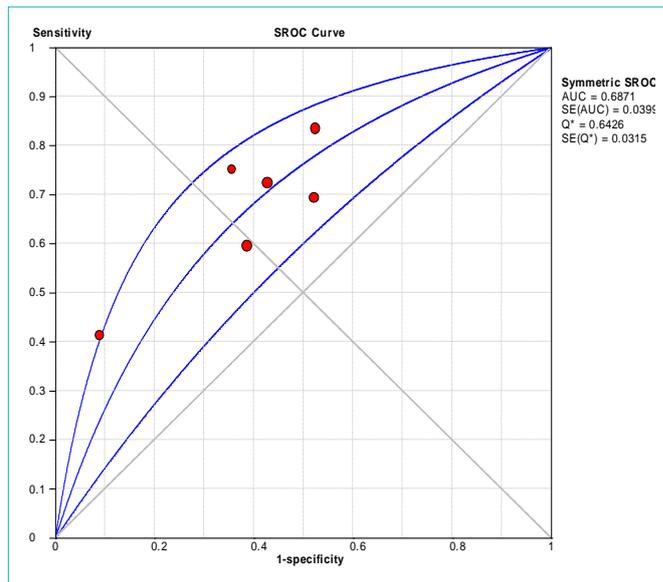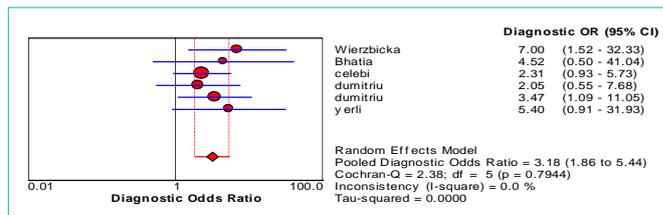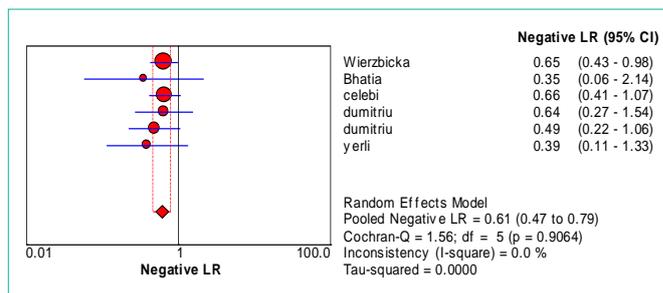

the pathology of the salivary gland mass is benign or malignant as lateral parotidectomy or extra capsular dissection could be applied for benign masses and total or radical parotidectomy along with neck dissection could be planned for malignant masses [12,13].

Salivary glands are superficial and most current imaging techniques such as B-mode sonography, Magnetic Resonance Imaging (MRI), And Computed Tomography (CT) is used as the imaging techniques in evaluating salivary gland masses. Although these modalities are used widely, they could not differentiate benign and malignant pathologies properly due to morphological overlaps between benign and malignant masses [14-16]. B-mode sonography is a time and cost-effective, easy to apply, and radiation free method which needs no contrast agent administration. However, most characteristics of benign masses overlap with malignant masses such as margin and echogenicity [17].

Computed Tomography (CT) and Magnetic Resonance Imaging (MRI) provide more information about the relationship surrounding tissues of the tumor or bony structures, but these modalities are time consuming, expensive and unavailable in all settings. Alternatively,

pre-operative cytological evaluation has been considered as the gold standard for evaluating salivary gland masses but its false negative and positive results is notable [18,19].

Palpation is a subjective method which gives information about the degree of firmness of the tumor as the malignant tumors are firmer than benign tumors.

By introducing sonoelastography in 1987 by Krouskop et al. evaluation of the elasticity features of the tissue and examination of changes in tissue hardness in response to external forces will be possible [20].

Nowadays, it is widely used for distinguishing benign and malignant pathologies in different tissues such as breast, thyroid, prostate, liver and lymph nodes [21-25].

In previous systematic reviews, summary sensitivities of sonoelastography in differentiating benign and malignant breast, thyroid, prostate and lymph nodes were 0.83, 0.92, 0.62, 0.74 and summary specificities were as follow: 0.84, 0.79, 0.9 and 0.9 [26-29].

We found that summary sensitivity and specificity of sonoelastography in differentiating benign and malignant parotid tumors were lower than the diagnostic accuracy of this method for pathologies of masses in other tissues. As sonography is operator dependent and elastography is a new method, its application in evaluating superficial glands such as tumors located in salivary glands. Maybe, more experience and precise definition of elastography method and application should be introduced to radiologist.

## References

- Pinkston JA, Cole P. Incidence rates of salivary gland tumors: results from a population-based study. *Otolaryngol Head Neck Surg.* 1999; 120: 834-840.
- Spiro RH. Salivary neoplasms: overview of a 35-year experience with 2,807 patients. *Head Neck Surg.* 1986; 8: 177-184.
- Yerli H, Eski E, Korucuk E, Kaskati T, Agildere AM. Sonoelastographic qualitative analysis for management of salivary gland masses. *J Ultrasound Med.* 2012; 31: 1083-1089.
- Gritzmann N, Rettenbacher T, Hollerweger A, Macheiner P, Hübner E. Sonography of the salivary glands. *Eur Radiol.* 2003; 13: 964-975.
- Schick S, Steiner E, Gahleitner A, Böhm P, Helbich T, Ba-Ssalamah A, et al. Differentiation of benign and malignant tumors of the parotid gland: value of pulsed Doppler and color Doppler sonography. *Eur Radiol.* 1998; 8: 1462-1467.
- Bradley MJ, Durham LH, Lancer JM. The role of colour flow Doppler in the investigation of the salivary gland tumour. *Clin Radiol.* 2000; 55: 759-762.
- Bhatia KS, Rasalkar DD, Lee YP, Wong KT, King AD, Yuen HY, et al. Evaluation of real-time qualitative sonoelastography of focal lesions in the parotid and submandibular glands: applications and limitations. *Eur Radiol.* 2010; 20: 1958-1964.
- Celebi I, Mahmutoglu AS. Early results of real-time qualitative sonoelastography in the evaluation of parotid gland masses: a study with histopathological correlation. *Acta Radiol.* 2013; 54: 35-41.
- Dumitriu D, Ducea S, Botar-Jid C, Baciut M, Baciut G. Real-time sonoelastography of major salivary gland tumors. *AJR Am J Roentgenol.* 2011; 197: 924-930.
- Dumitriu D, Ducea SM, Botar-Jid C, Baciut G. Ultrasonographic and sonoelastographic features of pleomorphic adenomas of the salivary glands. *Med Ultrason.* 2010; 12: 175-183.
- Wierzbička M, Kaluzny J, Szczepanek-Parulska E, Stangierski A, Gurgul E, Kopec T, et al. Is sonoelastography a helpful method for evaluation of parotid tumors? *Eur Arch Otorhinolaryngol.* 2013; 270: 2101-2107.
- Stennert E, Wittekindt C, Klusmann JP, Guntinas-Lichius O. New aspects in parotid gland surgery. *Otolaryngol Pol.* 2004; 58: 109-114.
- Klintworth N, Zenk J, Koch M, Iro H. Postoperative complications after extracapsular dissection of benign parotid lesions with particular reference to facial nerve function. *Laryngoscope.* 2010; 120: 484-490.
- Bozzato A, Zenk J, Greess H, Hornung J, Gottwald F, Rabe C, et al. Potential of ultrasound diagnosis for parotid tumors: analysis of qualitative and quantitative parameters. *Otolaryngol Head Neck Surg.* 2007; 137: 642-646.
- Ahuja AT, Evans R, Vlantis AC. Salivary gland cancer. In: Ahuja A, ed. *Imaging in head and neck cancer: a practical approach.* London: Greenwich Medical Media. 2003: 114-142.
- Som PM, Brandwein MS. Salivary glands: anatomy and pathology. In: Som PM, Brandwein M, eds. *Head and neck imaging.* St Louis, MO: Mosby. 2003: 2005-2033.
- Klintworth N, Mantsopoulos K, Zenk J, Psychogios G, Iro H, Bozzato A. Sonoelastography of parotid gland tumours: initial experience and identification of characteristic patterns. *Eur Radiol.* 2012; 22: 947-956.
- Zbären P, Guélat D, Loosli H, Stauffer E. Parotid tumors: fine-needle aspiration and/or frozen section. *Otolaryngol Head Neck Surg.* 2008; 139: 811-815.
- Howlett DC, Mercer J, Williams MD. Same day diagnosis of neck lumps using ultrasound-guided fine-needle core biopsy. *Br J Oral Maxillofac Surg.* 2008; 46: 64-65.
- Krouskop TA, Dougherty DR, Vinson FS. A pulsed Doppler ultrasonic system for making noninvasive measurements of the mechanical properties of soft tissue. *J Rehabil Res Dev.* 1987; 24: 1-8.
- Itoh A, Ueno E, Tohno E, Kamma H, Takahashi H, Shiina T, et al. Breast disease: clinical application of US elastography for diagnosis. *Radiology.* 2006; 239: 341-350.
- Lyshchik A, Higashi T, Asato R, Tanaka S, Ito J, Hiraoka M, et al. Cervical lymph node metastases: diagnosis at sonoelastography--initial experience. *Radiology.* 2007; 243: 258-267.
- Taylor LS, Rubens DJ, Porter BC, Wu Z, Baggs RB, di Sant'Agnese PA, et al. Prostate cancer: three-dimensional sonoelastography for in vitro detection. *Radiology.* 2005; 237: 981-985.
- Friedrich-Rust M, Ong MF, Herrmann E, Dries V, Samaras P, Zeuzem S, et al. Real-time elastography for noninvasive assessment of liver fibrosis in chronic viral hepatitis. *AJR Am J Roentgenol.* 2007; 188: 758-764.
- Teng DK, Wang H, Lin YQ, Sui GQ, Guo F, Sun LN. Value of ultrasound elastography in assessment of enlarged cervical lymph nodes. *Asian Pac J Cancer Prev.* 2012; 13: 2081-2085.
- Gong X, Xu Q, Xu Z, Xiong P, Yan W, Chen Y. Real-time elastography for the differentiation of benign and malignant breast lesions: a meta-analysis. *Breast Cancer Res Treat.* 2011; 130: 11-18.
- Bojunga J, Herrmann E, Meyer G, Weber S, Zeuzem S, Friedrich-Rus M. Real-Time Elastography for the Differentiation of Benign and Malignant Thyroid Nodules: A Meta-Analysis. *THYROID.* 2010; 20: 1145-1150.
- Teng J, Chen M, Gao Y, Yao Y, Chen L, Xu D. Transrectal sonoelastography in the detection of prostate cancers: a meta-analysis. *BJU Int.* 2012; 110: 614-620.
- Ying L, Hou Y, Zheng HM, Lin X, Xie ZL, Hu YP. Real-time elastography for the differentiation of benign and malignant superficial lymph nodes: a meta-analysis. *Eur J Radiol.* 2012; 81: 2576-2584.